




z-Logg.com


Specification & Configuration	
Device Name:	z1HT
Device Type:	Multi-use High Temp.
Serial Number:	HTE50001
Time Zone	GMT:-5 DST
Firmware Version:	5.04D
Software Version:	1.24.12 Admin
Trip Number:	4
Trip duration:	015d 19h44m00s
Temp. Unit:	Celsius
Temp. Range:	-40 to +130°C
Battery:	3.29V - 100%
Total Records:	1474
Sampling Rate:	00:01:00
Start Delay:	0 sec
Start Time:	24/05/24 16:50
Stop Time:	Parameter not set



Alarms (Time above / below Alarms)				
Type:	Temp.	Consecutive	Total	Out of Spec.
EH:	not set			
H:	not set			
L:	not set			
EL:	not set			

Summary / Statistics		File Created at: 25/05/24 17:18:07	
Maximum Temperature:	+30.69°C	Status:	Recording
Minimum Temperature:	-18.53°C	Trip Duration:	2d 01:07:00
Average Temperature:	+18.91°C	Time within Spec:	2d 01:07:00
Mean Kinetic Temp:	+44.85°C	Started Time:	24/05/24 16:45:18
Started by:		Memory Used:	6% 2948/45568
Stopped by:			

Description: Default Settings

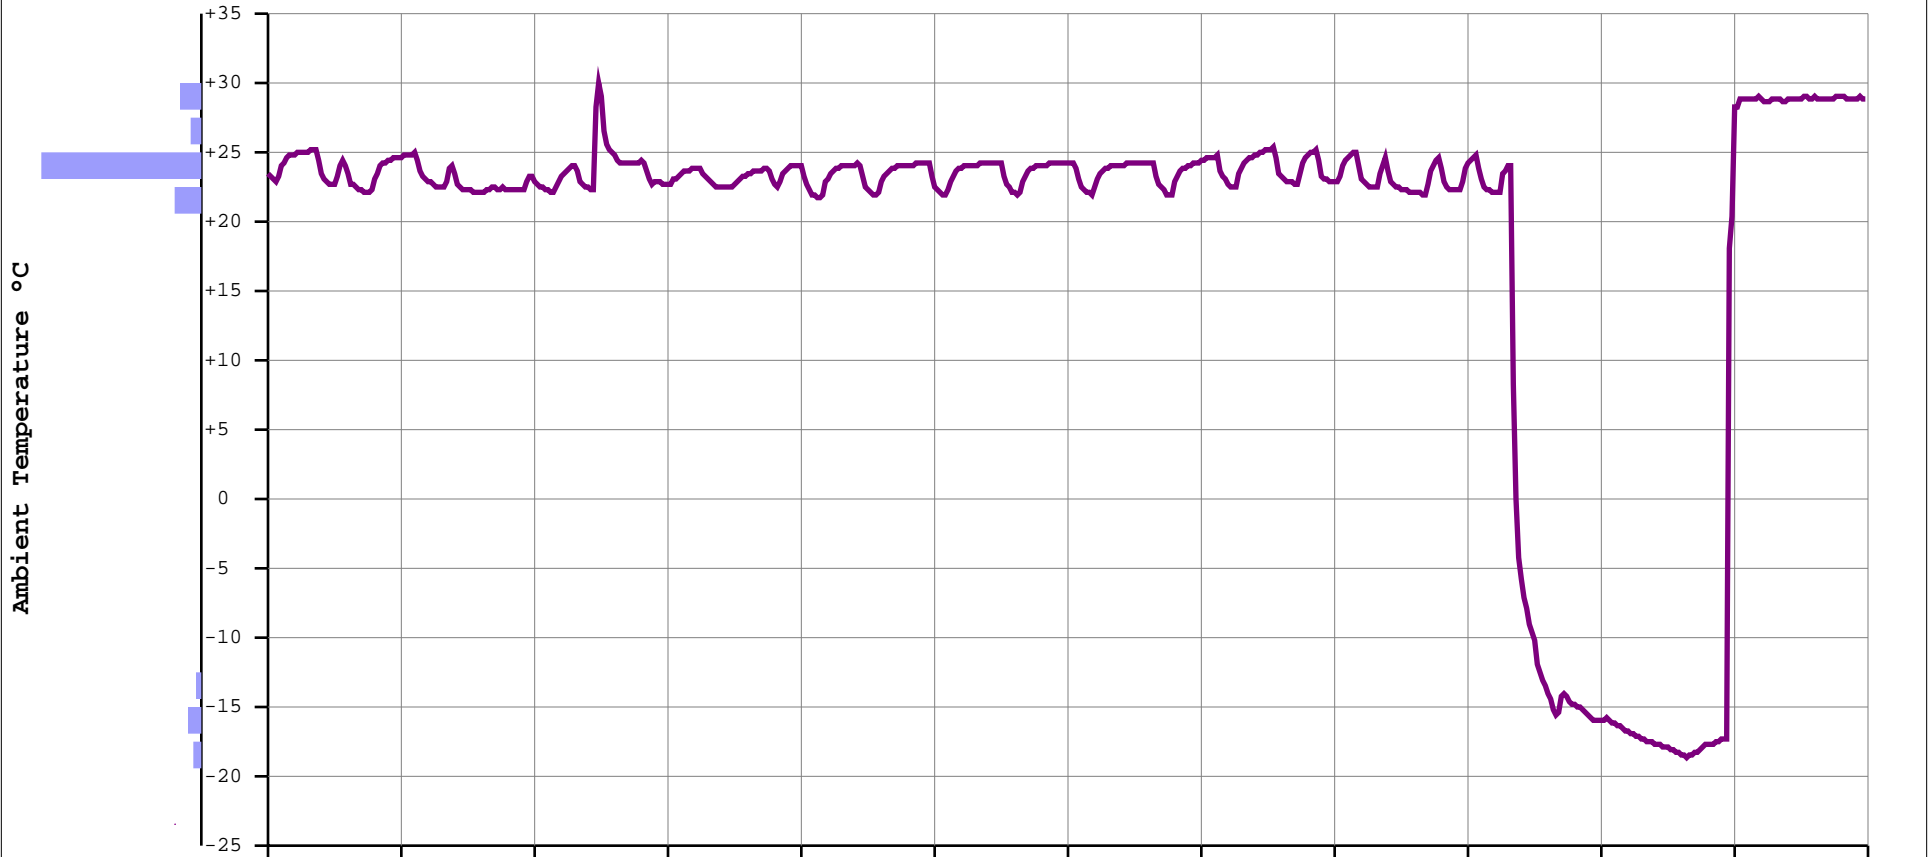

Max. #912	16:45:18	18:48:01	20:50:45	22:53:29	00:56:12	02:58:56	05:01:40	07:04:23	09:07:07	11:09:51	13:12:34	15:15:18	17:18:02
+22.5/+25.0°C	24/05/24	24/05/24	24/05/24	24/05/24	25/05/24	25/05/24	25/05/24	25/05/24	25/05/24	25/05/24	25/05/24	25/05/24	25/05/24

#Readings

Time/Date (dd/mm/yy)


Notes:

This z1HT with an accuracy of +/-0.2°C from -40°C to +125°C (-40°F to +257°F) and a resolution of 0.01°C (°F). Statement of accuracy: #HTE50001



z-Logg.com


Specification & Configuration	
Device Name:	z1HT
Device Type:	Multi-use High Temp.
Serial Number:	HTE50001
Time Zone	GMT:-5 DST
Firmware Version:	5.04D
Software Version:	1.24.12 Admin
Trip Number:	4
Trips Remaining:	Multiple
Temp. Unit:	Celsius
Temp. Range:	-40 to +130°C
Battery:	3.29V - 100%
Total Records:	1474
Sampling Rate:	00:01:00
Start Delay:	0 sec
Start Time:	24/05/24 16:50
Stop Time:	Parameter not set



Alarms (Time above / below Alarms)				
Type:	Hum.	Consecutive	Total	Out of Spec.
EH:	not set			
H:	not set			
L:	not set			
EL:	not set			

Summary / Statistics		File Created at: 25/05/24 17:18:07	
Maximum Temperature:	+31.19°C	Status:	Recording
Minimum Temperature:	-18.06°C	Trip Duration:	1d 00:33:00
Average Temperature:	+19.01°C	Time within Spec:	1d 00:33:00
Started by:		Stopped Time:	25/05/24 17:18:02
Stopped by:			

Description: Default Settings

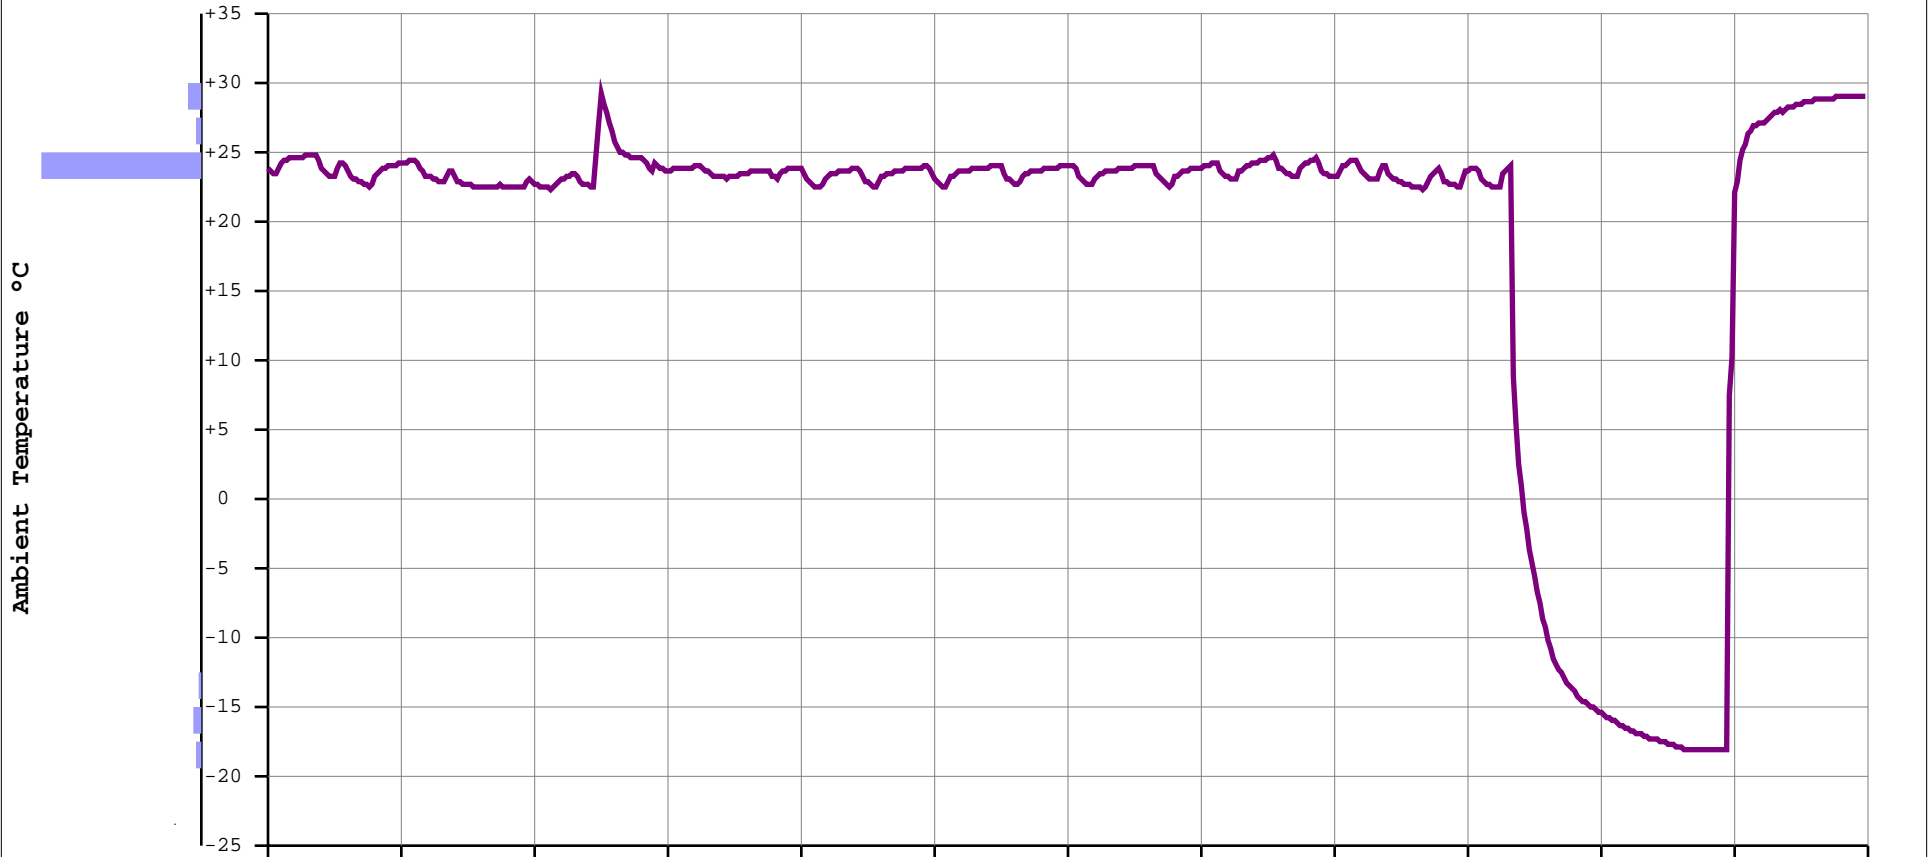

Max. #1123	16:45:18	18:48:01	20:50:45	22:53:29	00:56:12	02:58:56	05:01:40	07:04:23	09:07:07	11:09:51	13:12:34	15:15:18	17:18:02
+22.5/+25.0°C	24/05/24	24/05/24	24/05/24	24/05/24	25/05/24	25/05/24	25/05/24	25/05/24	25/05/24	25/05/24	25/05/24	25/05/24	25/05/24

#Readings

Time/Date (dd/mm/yy)

Notes:

This z1HT with an accuracy of +/-0.2°C from -40°C to +125°C (-40°F to +257°F) and a resolution of 0.01°C (°F). Statement of accuracy: #HTE50001